

## Registratie sensibiliteits testen

© Afdeling Revalidatie – Handtherapie Erasmus MC versie 2.0 2005

Naam \_\_\_\_\_


Datum test: \_\_\_\_\_

Geb dd. \_\_\_\_ - \_\_\_\_ - \_\_\_\_

Tester: \_\_\_\_\_

Diagnose: \_\_\_\_\_

Filament (SWF) nummer/ afstand mm (2PD) aangeven welke **WEL** gevoeld wordt

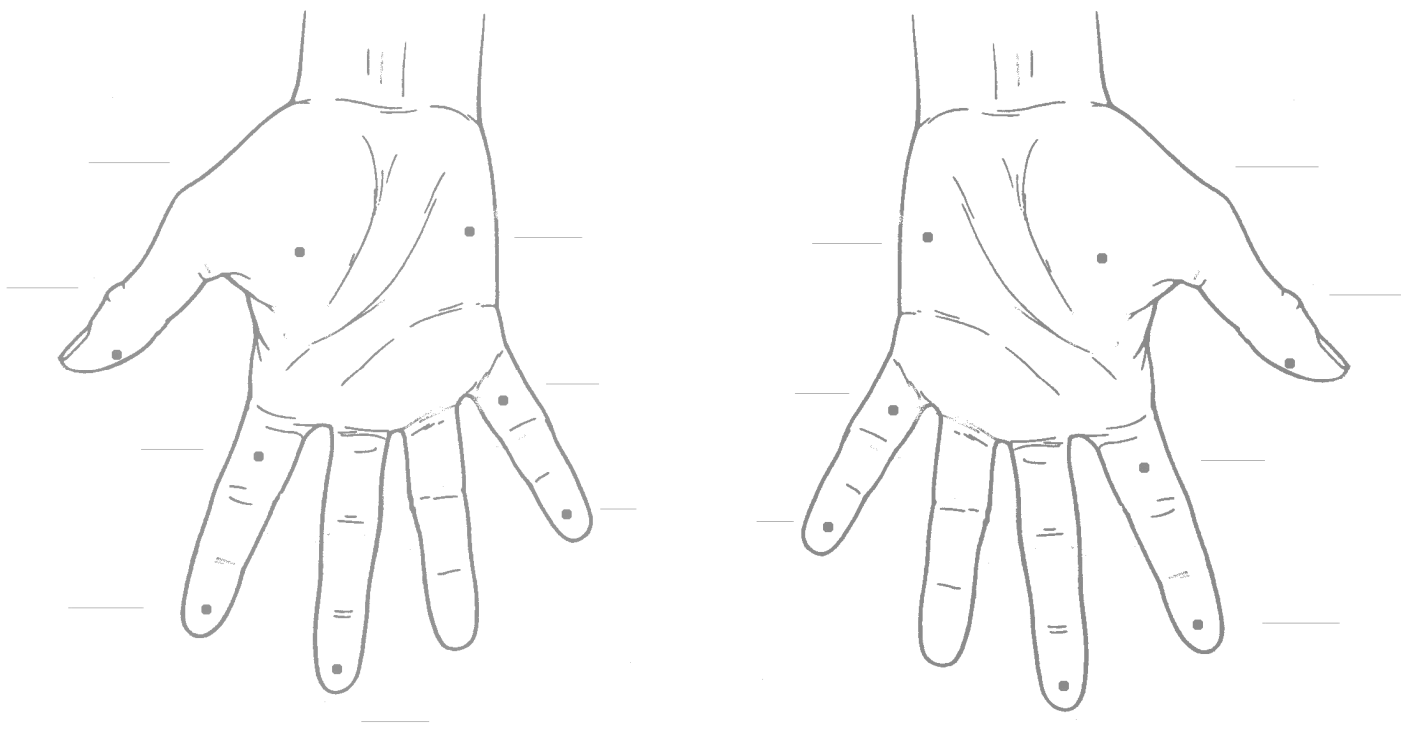

<b>Filament</b>	<b>force, gm</b>	<b>Interpretations &amp; Marking Numbers</b>	<b>appliceren</b>
A (Green)	0.05	Normal (2.83)	3x
B (Blue)	0.20	Residual Texture (3.61)	3x
C (Purple)	2	Residual Protective Sensation (4.31)	
D (Red)	4	Loss of Protective Sensation (4.56)	
E (Orange)	300	Residual Deep Pressure (6.65)	